



REF **SupermarketVR**

CE Class I Medical Device

User manual

Distribution mode

Available for direct download at
<http://virtualisvr.com/espace-client/>
Use under licence



Avenue de l'Europe - 34830 CLAPIERS - Tel. 09 80 80 92 91



DESCRIPTION

SUPERMARKETVR software is an immersive 3D simulation based on virtual reality technology, i.e. it allows a person to be immersed in an artificial digitally created world. **SupermarketVR** is a software used for reintegrating Activities of Daily Living, memory training and multi-tasking.

INDICATIONS

Assessment and rehabilitation of cognitive disorders (memorization, executive functions...)

Situational rehabilitation of an upper limb (shoulder) or of the lumbar spine.

CONTRAINDICATIONS

Epileptic patients, children under 15 years of age, pregnant women.

FOR USE BY

Healthcare professionals: Physiotherapists; Occupational therapists; Neuropsychologists; ENT doctors; Neurologists; PMR doctors (physical medicine and rehabilitation), etc.

Research Centers: CNRS, CHU, INSERM, etc.

WARNINGS AND CAUTIONS

During sessions, stay close to the patient in order to anticipate any loss of balance or discomfort caused by the use of virtual reality.

Define a working area of about 3m² to allow for risk-free movements.

Take a 10 to 15 minute break every 30 minutes of use.

Potential adverse effects are those due to software, i.e. vomiting, malaise, dizziness, syncope

The accessories required to use the software may emit radio waves that can interfere with the operation of nearby electronic devices. If you have a pacemaker or other implanted medical device, do not use the product until you have taken advice from your doctor or the manufacturer of your medical device.



Any serious incident should be notified in writing to qualite@virtualisvr.com



Table of Contents

- 1. GENERAL..... 3
 - 1.1. Advice for use 3
 - 1.2. Hardware and minimum configuration requirements 3
- 2. USE OF PATIENT MANAGEMENT..... 4
- 3. SUPERMARKET..... 6
 - 3.1. Start interface..... 6
 - 3.2. Module field of application 7
 - 3.3. Installing the patient 7
 - 3.4. Session settings 7
 - 3.5. Shortcuts 9
 - 3.6. Data processing 10



1. GENERAL

1.1. Advice for use

This type of re-education must be undertaken progressively, especially in Virtual Reality where the stimulation is much more "powerful" than the traditional optokinetic stimulators.

These stimulations have the potential to cause certain disorders: Vasovagal syncope, epileptic seizures, migraines, etc. (Despite a test phase on more than 2000 patients. Similarly to previous generation optokinetics, caution is required)

The contraindications are identical: Mainly epilepsy and migraines.

As postural reactions can be spectacular, it is VERY STRONGLY advised to place patients in a safe environment and to stay close to them throughout the session.

It is also recommended to increase the duration and intensity of the stimulation very gradually, after an initial short session to make sure of patients' tolerance to this type of stimulation.


Virtualis declines any liability for any disorders suffered by patients during or after use of its software.

1.2. Hardware and minimum configuration requirements

Hardware required to use the system:

- VR Ready PC
- VR System: HTC VIVE, HTC VIVE Pro or compatible system
- Lighthouse bases (HTC VIVE tracking)
- HTC VIVE Controller
- XBOX 360 Controllers
- USB HUB

In order to install and use our virtual reality applications, we recommend a configuration equal to or higher than the system requirements:

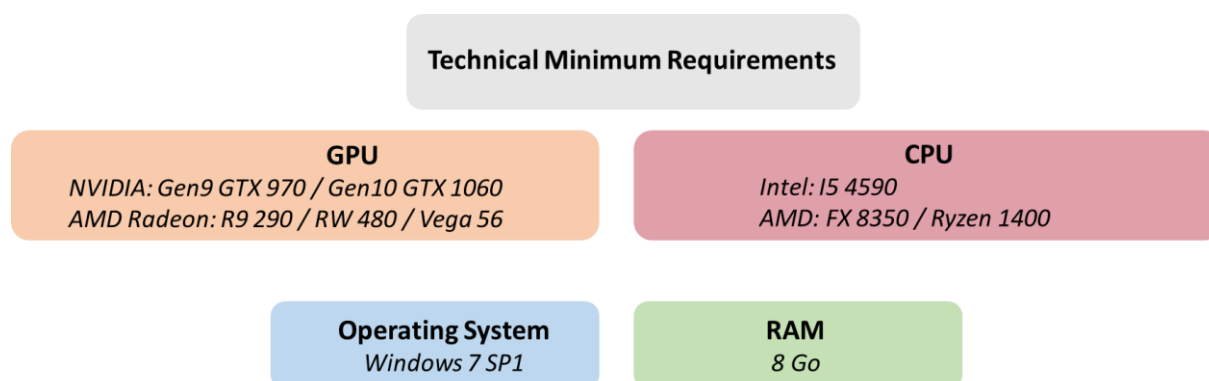




2. USE OF PATIENT MANAGEMENT

Once connected to the Patient Management software, you arrive on the home page. It is from this home page that you will be able to start your VR software as well as the other Patient Management functions.


The software can be grouped according to criteria such as "Assessment" or "Re-education" and then by pathology type: Neurology, Balance, Functional or Travel sickness.

You can start or switch from one software to another from the home page by clicking the corresponding "Start" or "Protocols" button.

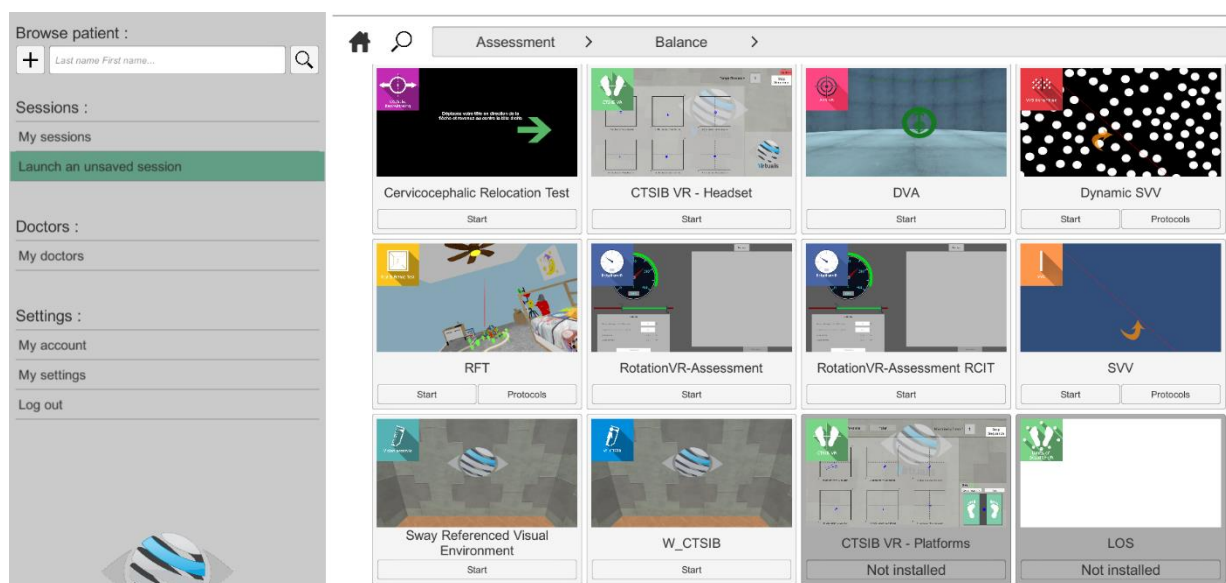


Some software can be started either in **manual mode**, by directly clicking the "Start" button, or in **protocol mode** by clicking the "Protocols" button.

The **manual mode** allows users to choose the settings for each environment. The **protocol mode** offers several sessions with different difficulty levels to test and gradually accustom patients to the VR environment.

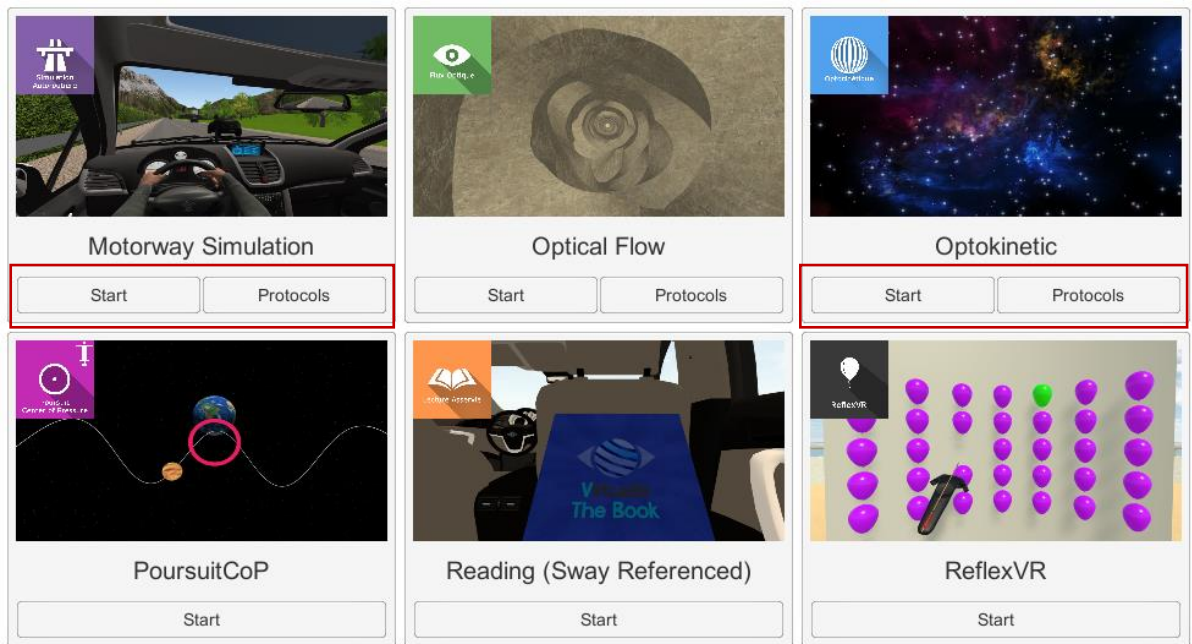


Software that is not part of your subscription package is greyed out. If you want to use it, please contact our sales department.

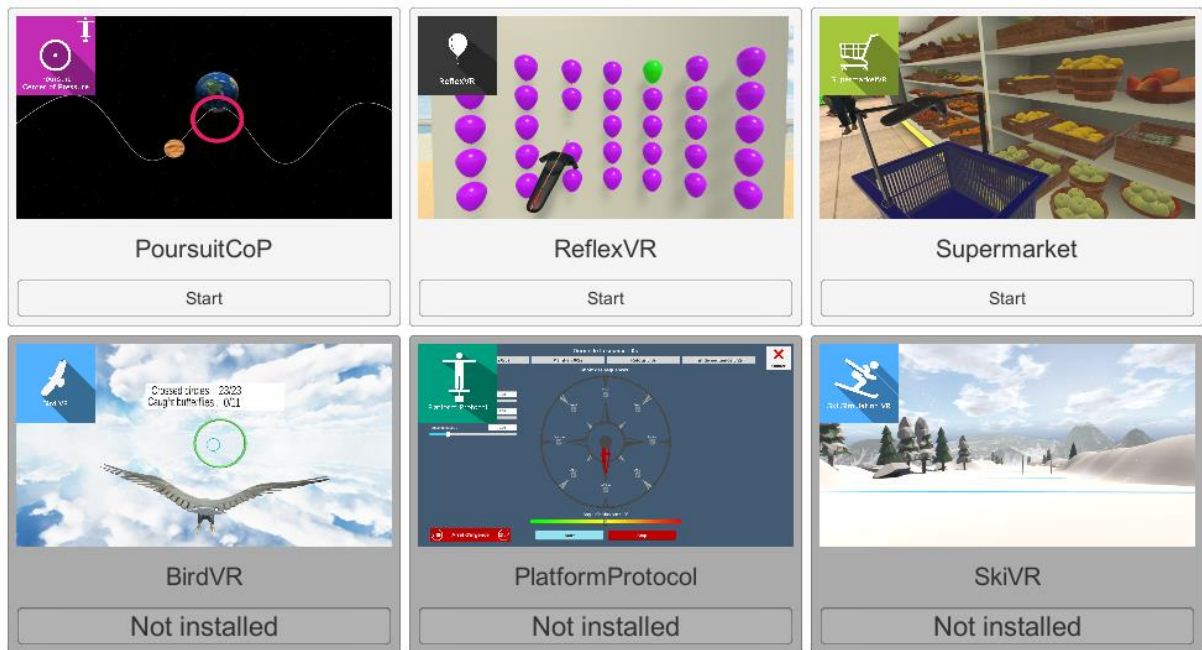



3. SUPERMARKET

3.1. Start interface

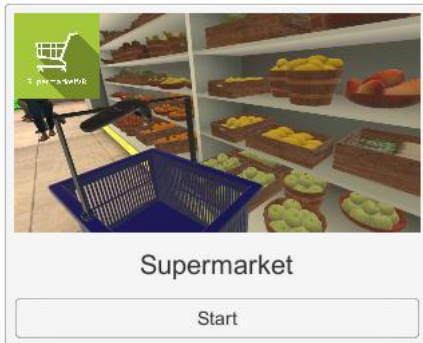


When starting the software in **manual mode** ("Start" button) from Patient Management, the software is opened in a start interface consisting of a module selection menu on the left, a set up area on the right, and an action area at the bottom right.

Depending on the module selected in the left menu, the set up area shows the various possible settings/information.

The general Patient Management menu can be accessed from the start interface by simply clicking the "Back" button located in the action area, or by pressing the "escape" key on the keyboard.

The module is launched by simply clicking the "Start" button in the action area.

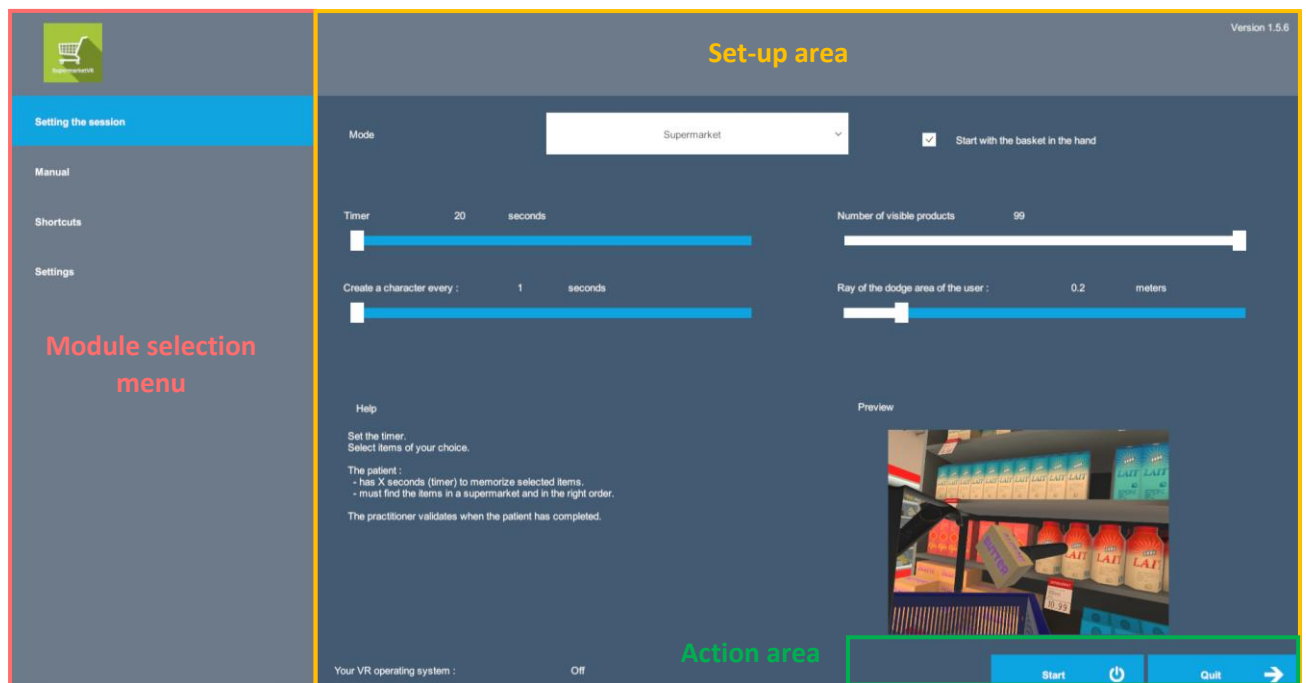

Once this button is pressed, the module starts by taking into account the specified settings. You also have the possibility to modify some settings when the module has been launched, using the mouse.

The Start/Quit buttons allow the environment to be played back or stopped entirely to adapt the experience to the patient's sensations.



3.2. Module field of application

Complete simulation of everyday life activities (decision-making, economy of movement, memorization, travel strategy).

3.3. Installing the patient


Patients standing upright with sufficient space around them for a few small movements
(3m x 3m)

3.4. Session settings

The variable settings for this module are as follows:

Timer

Time given to patients to memorize the objects to be found.

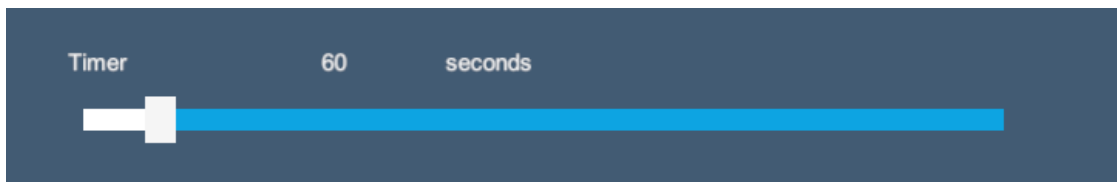

Number of visible products

Used to select the number of products displayed using the cursor

Character creation


Used to select the frequency at which characters appear

Dodge area radius

Used to determine the distance between the user and the other characters

Selected articles

Selection of the items that patients will have to find in order. To select an object, drag it to the left area or double-click it. Random object selection can be used using the "Random" button by specifying the number of products to be selected.

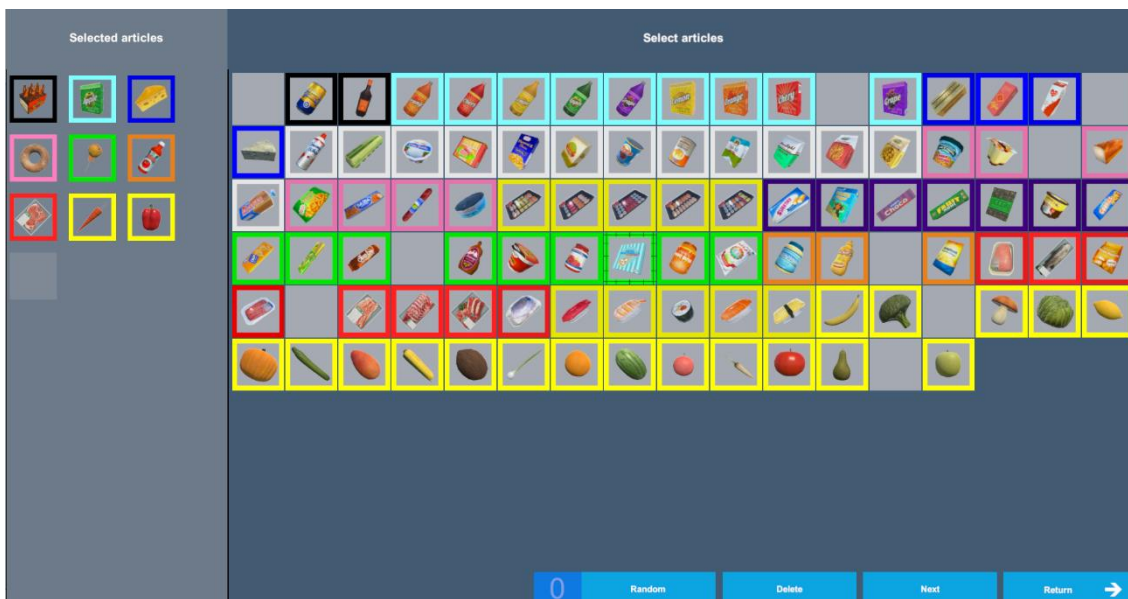


Patient interface

Users can use the controller in each environment (color code) to fetch the required articles.

Score


At the end of the exercise, users will get a score showing their success relative to the selected articles.

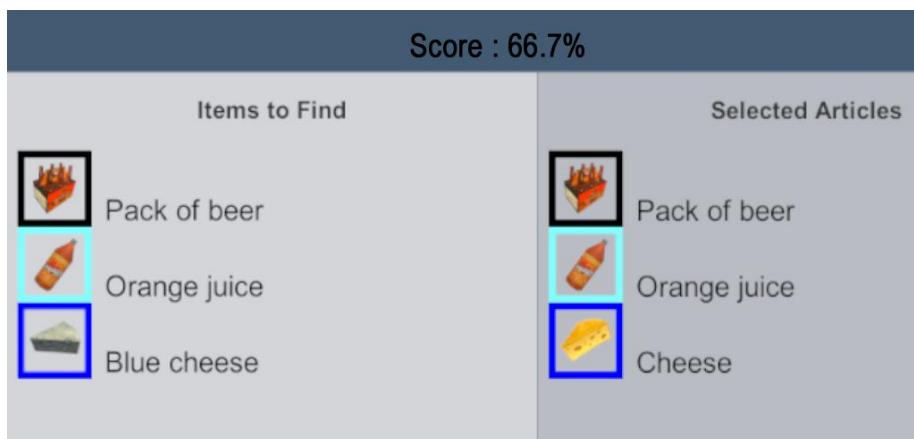

3.5. Shortcuts

Keyboard, joystick or controller shortcuts can be accessed in two ways:

- on the "Shortcuts" tab available at the start interface level
- within the module, by clicking on the joystick icon in the upper right corner of the screen

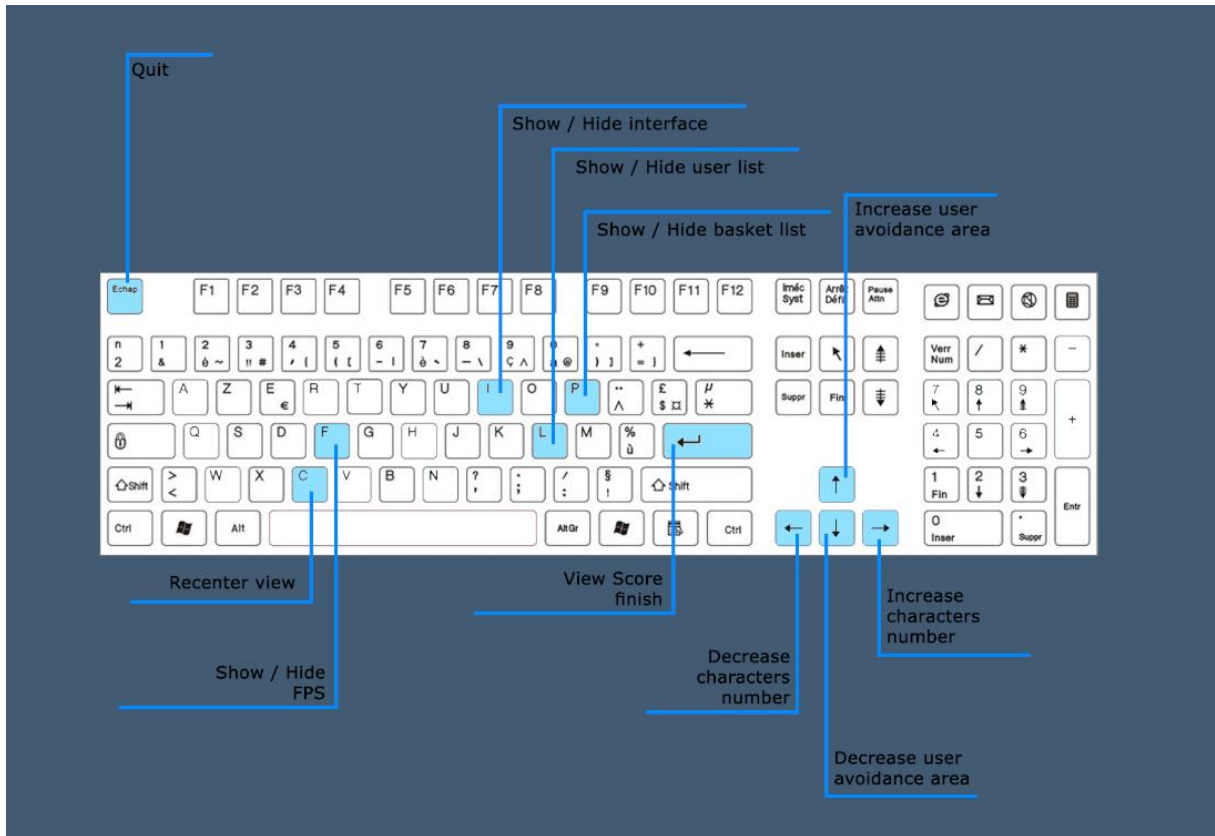



Teleportation: Use the controller to aim at the place you want to go to and then press this button to teleport



Fast teleportation: Use the controller to aim at a sign to teleport to the associated aisle. Touch an item using the controller and then press the button to select it

3.6. Data processing

Data retrieval and analysis uses the Patient Management software.